



1947

1947 VACUUM-GAUGE TUBE

PIRANI TYPE


DATA

General:

Filament, Platinum Iridium:
 Voltage (Approx.) 10 dc volts
 Current (Varies with Gas Pressure) 70-100 ma.
 Resistance between base pins No.1 & No.2 under vacuum better than 3×10^{-5} mm of mercury 135.8 ohms
 Maximum Overall Length (including tubulation) 7-9/16"
 Maximum Diameter 1-3/16"
 Bulb T-9
 Tubulation 7/32" Diameter Soft Glass, Corning Code 001 Lead
 Mounting Position Any
 Base Small-Shell Small 4-Pin

BOTTOM VIEW

- Pin 1 - Filament
- Pin 2 - Filament
- Pin 3 - No Connection
- Pin 4 - Internal Connection - Do Not Use



R - Series Filament-Calibrating Resistor in base of tube


Maximum Ratings, Absolute Values:

FILAMENT VOLTAGE 16 max. volts

Calibration for 1947 in Accompanying Circuit:

See curve on following sheet.

PIRANI GAUGE BRIDGE CIRCUIT

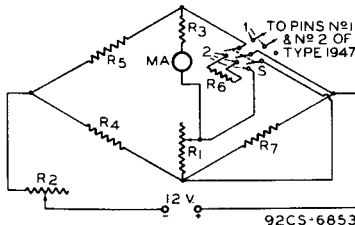


- 92CS-6853
- R1: 50 Ohms R3 + METER: 15 Ohms R6: 120.7 Ohms
 - R2: 25 Ohms R4 R5: 10 Ohms each R7: 135.8 Ohms
- STEP 1: With switch S in position 2, adjust R2 so that meter reads 2.5 milliamperes.
- STEP 2: With switch S in position 1, and with dry air at atmospheric pressure in the 1947, adjust R1 so that meter reads 5.0 milliamperes.
- STEP 3: With no further adjustments and with switch S in position 1, proceed to use gauge.

1947



1947

VACUUM-GAUGE TUBE

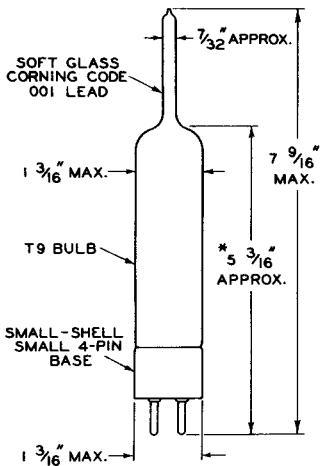

* MEASURED FROM END OF BASE PINS TO BULB-TOP LINE AS DETERMINED BY RING GAUGE OF $\frac{1}{2}$ " I.D.

92CS-6816



1947

1947

CALIBRATION CURVE FOR USE WITH CIRCUIT ON DATA PAGE

GAS = DRY AIR
TO CONVERT MM TO MICRONS,
MULTIPLY VALUES BY 1000.

